BODYSTEEL & SILVER CO.,LTD
63 Moo 5, Soi Wat Bang-Co Yaek Rong-Foam, Kanchanaphisek Road
Bang Ma-Nang, Bang Yai, NONTHABURI 11140 THAILAND
☎ 66 2-1505999 66-2-1505990
sales@steelandsilver.com

EO STERILIZATION
Quality Control Report

Date : 7-Aug-2026

LOT : 1266	**STERILIZATION DATE : 30-July-2026**	**EXPIRE DATE : 30-July-2031**

QC REPORT :


PASS as the test result has been shown as pictures below.

BIOLOGICAL INDICATORS :

The EZTest indicator is placed in a suitable test pack which is representative of the load. The load is then processed as usual.

After sterilization the chemical indicator ring on the label changes from blue to brownish when exposed to Ethylene Oxide (EO gas). This distinguishes exposed from unexposed units (it does not indicate acceptable sterilization).

After the incubation period of 48 hours, the appearance of a yellow color indicates bacterial growth. No color change indicates adequate sterilization.

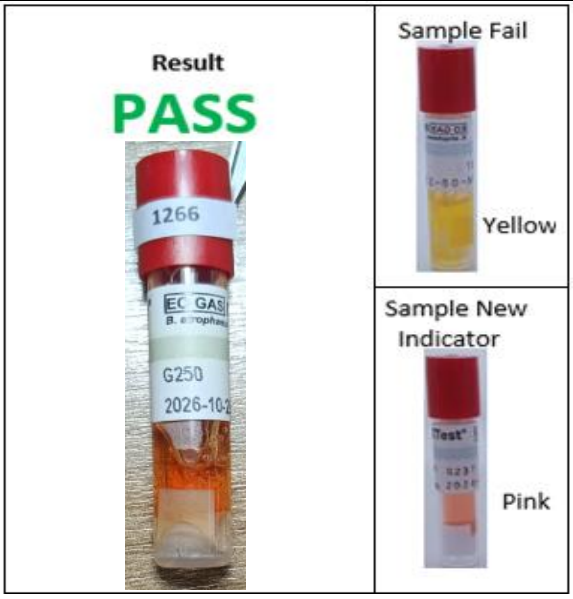

Quality Assurance By:

Date: 7-Aug-2026

STEEL AND SILVER CO.,LTD. BODY

lot 1266

Welcome use sangiang medical equ
Ethylene oxide sterilize
Ster T: 50 ℃
Ster H: 55 %
Steritime: 6h 0min
Cleantimes: 6 pic
Clean P: 0 kPa
Cleantime: 15 min

	T ℃	P kPa	H %	time
Start:	24.1	-0.3	3.2	14:20
Water:	24.2	-0.3	35.0	14:21
Vacuu:	24.2	-5.0	35.9	14:21
Prhet:	35.0	-3.3	35.2	14:39
KHeat:	34.9	-2.7	35.0	14:48
Vacuu:	34.0	-60.0	35.4	14:55
KeepP:	40.1	-59.2	35.7	15:03
Inta:	40.2	-5.0	35.5	15:09
Vacuu:	38.5	-60.0	35.5	15:15
Humid:	40.3	-58.5	35.7	15:25
KHum:	38.0	-57.1	35.7	15:55
Dost:	37.4	-58.5	35.2	16:08
Rst:	37.6	-47.4	35.8	16:08
Diffu:	37.2	-24.6	35.4	16:18
Heat:	50.1	-15.0	35.9	16:57
Steri:	50.0	-15.0	35.9	16:57
Steri:	52.2	-13.5	35.1	17:07
Steri:	51.8	-13.1	35.1	17:17
Steri:	50.7	-12.7	35.9	17:27
Steri:	50.3	-12.2	35.3	17:37
Steri:	50.2	-11.7	35.5	17:47
Steri:	50.2	-11.4	35.7	17:57
Steri:	50.3	-11.0	35.7	18:07
Steri:	50.1	-10.7	35.5	18:17
Steri:	50.4	-10.4	35.7	18:27
Steri:	50.0	-10.1	35.1	18:37
Steri:	50.4	-9.8	35.7	18:47
Steri:	50.1	-9.5	35.1	18:57
Steri:	50.4	-9.3	35.9	19:07
Steri:	50.2	-9.1	35.1	19:17
Steri:	50.3	-8.8	35.5	19:27
Steri:	50.4	-8.6	35.1	19:37
Steri:	50.1	-8.5	35.3	19:47
Steri:	50.4	-8.3	35.1	19:57
Steri:	50.1	-8.1	35.5	20:07
Steri:	50.4	-8.0	35.9	20:17
Steri:	50.0	-7.8	35.9	20:27
Steri:	50.4	-7.7	35.5	20:37
Steri:	50.2	-7.6	35.3	20:47
Steri:	50.2	-7.5	35.3	20:57
Steri:	50.2	-7.4	35.5	21:07
Steri:	50.2	-7.3	35.5	21:17
Steri:	50.3	-7.1	35.7	21:27
Steri:	50.0	-7.0	35.5	21:37
Steri:	50.3	-7.0	35.3	21:47
Steri:	50.2	-6.8	35.1	21:57
Steri:	50.3	-6.8	35.1	22:07
Steri:	50.4	-6.7	35.3	22:17
Steri:	50.1	-6.7	35.7	22:27
Steri:	50.3	-6.6	35.7	22:37
Steri:	50.1	-6.5	35.7	22:47
Steri:	50.2	-6.5	35.8	22:57

Clean Process

1th :	51.0	-37.7	23:24
2th :	50.6	-40.1	23:54
3th :	50.5	-40.2	00:25
4th :	50.5	-40.7	00:56
5th :	50.4	-40.5	01:26
6th :	50.4	-40.4	01:57
Inta:	50.4	-36.2	35.1 01:58
End:	50.4	-36.2	35.1 01:58

Sterilization Completed
Steril Time: 11h30min
Usecount: 00250
Date: 2026-7-30
Number: 500000450051
Operator:

Protocol: